



C O N V E N I E N C E

Easy to use: just dip then read

No timing required: control line indicates read time

Temperature strip included on kit collection cup

Clear collection cup: allows for visual integrity check

Results ready in 3-5 minutes

P E R F O R M A N C E

Test administrator maintains possession of test device

Built-in procedural control

Results stable for up to one hour

>99% correlation to GC/MS at 95% confidence level

Colloidal gold technology

= superior sensitivity, accuracy & precision

Tested for cross-reactivity against over 600 compounds

SAMHSA cut-off levels

US FDA 510(k) cleared for commercial distribution

F L E X I B I L I T Y

2 to 10 drugs per panel

15 drugs assays to choose from

Available as part of a kit or test card only

Custom configurations available

Multiple cut-off options for certain drugs

Low volume procedure - as little as 100 µL

Compatible with Rapid Reader® result interpretation

and data management system

T R A I N I N G

Web based training with certification

Onsite training

T E C H N I C A L S U P P O R T

Available 24/7/365



AMP
amphetamines
1000ng/mL

BAR
barbiturates
300ng/mL

BZO
benzodiazepines
300ng/mL

BUP
buprenorphine
12.5ng/mL

COC
cocaine
150 & 300ng/mL

MDMA
ecstasy
1000ng/mL

MTD
methadone
300ng/mL

METH
methamphetamines
1000ng/mL

NIC*
nicotine
200ng/mL

OPI
opiates
300 & 2000ng/mL

OXY
oxycodone
100ng/mL

PCP
phencyclidine
25ng/mL

PPX
propoxyphene
300ng/mL

THC
marijuana
50ng/mL

TCA
tricyclic
antidepressants
1000ng/mL

*Nicotine is not
USA 510(k) cleared

ACCURACY

An Evaluation of Non-Instrumented Drug Test Devices



Substance Abuse and Mental Health Services Administration (SAMHSA)

Division of Workplace Programs

The purpose of this study was to evaluate the performance of 15 point of collection drug test devices.

The results were compared to the Syva EMIT assays run on a Behring Diagnostics ETS analyzer.

The Rapid Drug Screen® (RDS®) was ranked the most accurate multi-drug device for all drugs when compared to GC/MS.

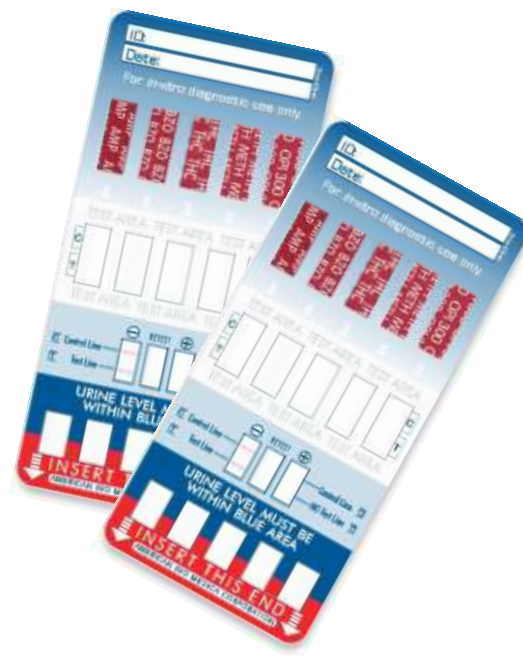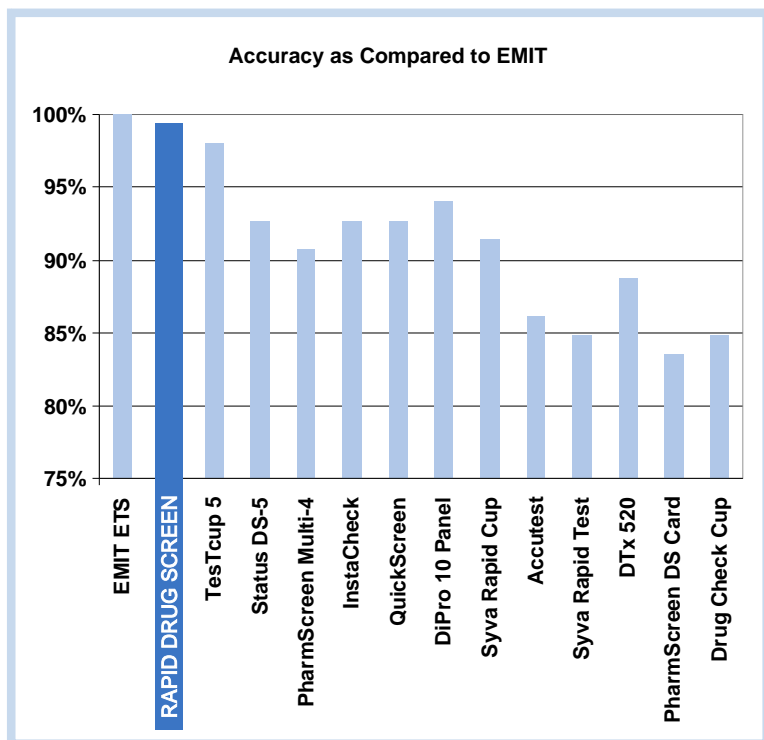

Department of Health and Human Services 1999

Note: The entire study may be found at:

<http://www.workplace.samhsa.gov/resourcecenter/r409.htm>



1 2 2 S M I T H R O A D , K I N D E R H O O K , N E W Y O R K 1 2 1 0 6

W W W . A B M C . C O M ■ 8 0 0 . 2 2 7 . 1 2 4 3 ■ 5 1 8 . 7 5 8 . 8 1 5 8